

MAN436

**Models 76870
76870V**

Adjustable Arm Subject's Chair Setup and User's Manual













3700 Sagamore Pkwy N
Lafayette, IN 47904
Tel: (765) 423-1505

info@lafayetteinstrument.com
www.lafayetteinstrument.com

Adjustable Arm Subject's Chair

Parts Included (not actual size)

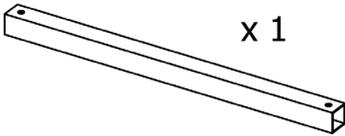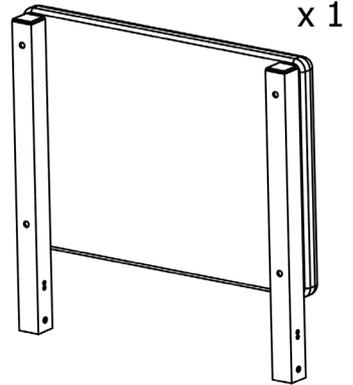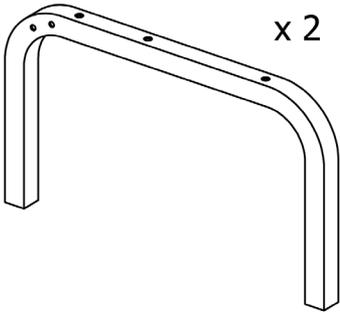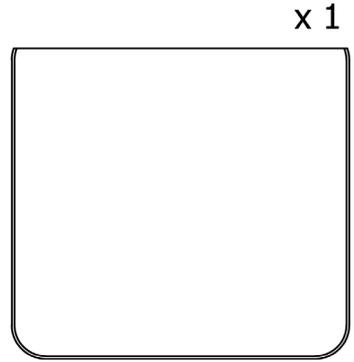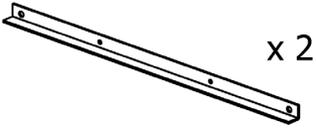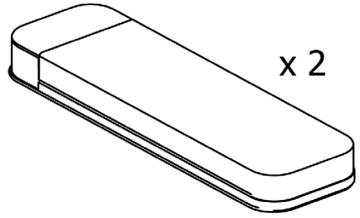

Setup and User's Manual

Part A: qty 4



Part B: qty 6



Part C: qty 6



Part D: qty 4




Part E: qty 12



Part F: qty 4





Part G: qty 2



Part H: qty 2




Part I: qty 6




Part J: qty 2



Part M: qty 4



Part N: qty 2



Part P: qty 4

- A. 5/16"-18 Heavy Hex Nut
- B. 3/8"-16 Hex Nut
- C. 1/2" Split Lock Washer
- D. 5/16" Split Lock Washer
- E. 1/4"-20 x 1" Socket Head Cap Screw
- F. 1/4"-20 x 1/4" Button Head Socket Cap Screw
- G. 3/8" Shoulder x 3" Long, 5/16"-18 Thread

- H. 3/8" Shoulder x 1-1/2" Long, 5/16" Thread
- I. 1/2" Shoulder x 1-1/2" Long, 3/8"-16 Thread
- J. 1/4" Diameter x 2" Clevis and Cotter Pin
- M. 1.58" x 0.75" Strut Channel Nut - 1/4"-20 Thread
- N. 3" Rubber Knob, 1/4"-20 Stud
- P. 1-3/4" Knob, 1/4"-20 x 1/2" Stud

Tools Included (not actual size)




3/16" Hex Key



1/4" Hex Key



9/16" Wrench



5/32" Hex Key


Setup Instructions

Step 1

Required

- Part E: qty 4
- 3/16" Hex Key

1. Attach the angles to the seat as shown. Do not tighten completely.

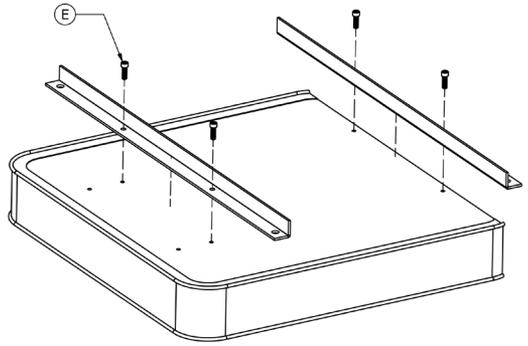


Step 2

Required

- Part B: qty 6
- Part C: qty 6
- Part I: qty 6
- 9/16" Wrench
- 1/4" Hex Key

2. Place the seat cushion upside down on the floor.
3. Attach the seat cushion to the angle brackets. Make sure the thicker portion is furthest away from the two holes in the sides of the legs.
4. Attach the angle brackets and tube to the legs. Do not tighten completely.

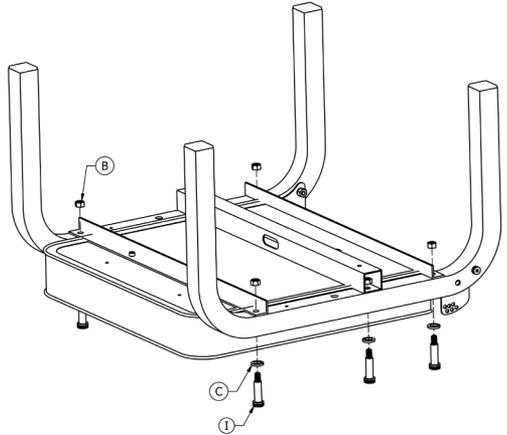


Step 3

Required


- Part M: qty 4
- Part N: qty 2
- Part P: qty 2

5. Attach the nuts to the handles as shown. The large handle goes on the L shaped piece. Do not tighten the handles.

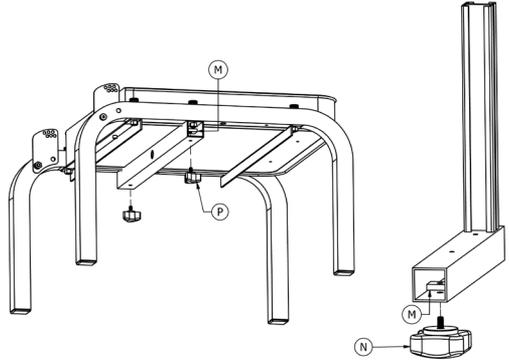

Step 4

6. Gently slide the channel into the tube and tighten the handle.

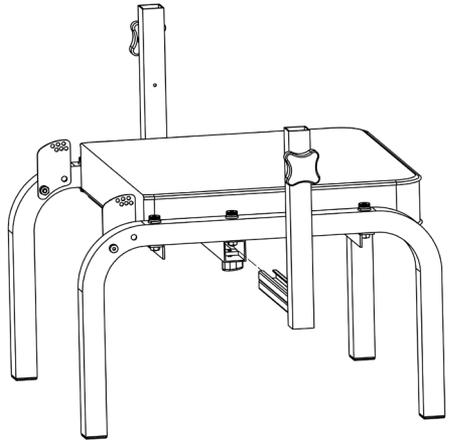


Adjustable Arm Subject's Chair

Step 5

Required



- Part A: qty 2
 - Part D: qty 2
 - Part J: qty 2
 - 9/16" Wrench
 - 3/16" Hex Key
7. Attach the back piece as shown. Put the clevis pin through the plate and back tube and secure in place with the cotter pin.
 8. Make sure that everything is straight and tighten everything down from previous steps.

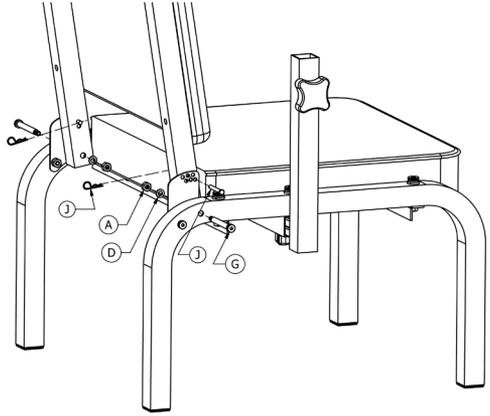

Step 6

Required

- Part P: qty 2
 - Part F: qty 4
 - 5/32" Hex Key
9. Slide out the arms approximately as shown and attach the support plate with the screws and the small handles.

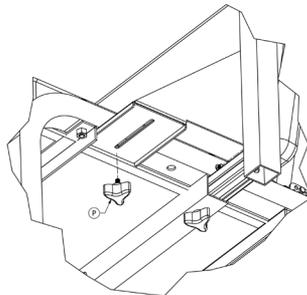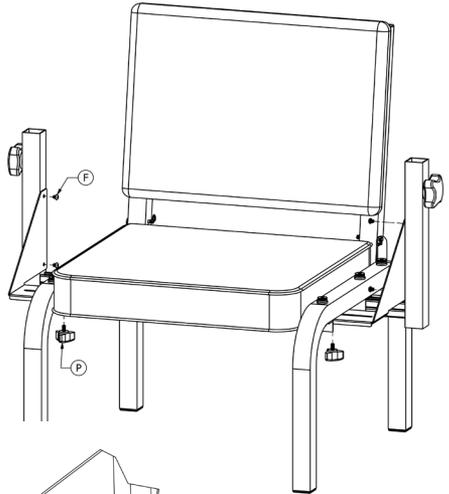


Step 7

Required


- Part E: qty 8
- 3/16" Hex Key

10. Attach the arm cushions to the plates.

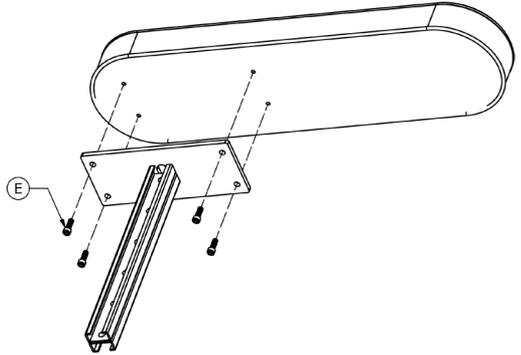

11. Slide the arms into the arm support tubes as shown. Turn the knob clockwise to tighten into place at desired height. The knobs only need to be loosened a little bit to reposition the arms.

WARNING: Always hold onto the arm cushions when loosening the height adjustment handle to avoid injury.

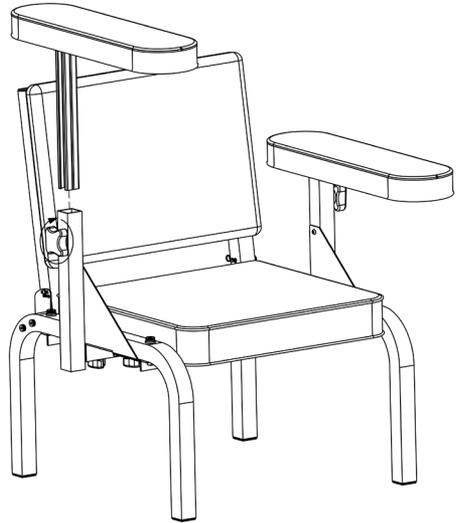

Terms and Conditions

Worldwide Headquarters

Lafayette Instrument Company
3700 Sagamore Parkway North
Lafayette, IN 47904, USA

Tel: (765) 423-1505

Fax: (765) 423-4111

sales@lafayetteinstrument.com

European Office

Tel: +44 1509 817700

Fax: +44 1509 817701

sales@campdeninstruments.com

Placing an Order

All orders need to be accompanied by a copy of your purchase order. All orders must include the following information:

- Quantity
- Part Number
- Description
- Purchase order number or method of pre-payment
- Tax status (include tax-exempt numbers)
- Shipping address for this order
- Billing address for the invoice we'll mail when this order is shipped
- Telephone number
- Email address
- Signature and typed name of person authorized to order these products

Exchanges and Refunds

No item may be returned without prior authorization from Lafayette Instrument Company and a Return Materials Authorization (RMA#) number which must be affixed to the shipping label of the returned goods. The merchandise should be packed well and insured for the full value. Unopened merchandise may be returned prepaid within thirty (30) days after receipt of the item and in the original shipping carton. Collect shipments will not be accepted. Product must be returned in saleable condition, and credit is subject to inspection of the merchandise.

Repairs

Instrumentation may not be returned without first receiving a Return Materials Authorization Number (RMA). When returning instrumentation for service, please contact Lafayette Instrument to receive an RMA number. Your RMA number will be good for 30 days. Address the shipment to:

Lafayette Instrument Company
RMA# XXXX
3700 Sagamore Parkway North
Lafayette, IN 47904, USA.

Shipments cannot be received at the PO Box. All items should be packed well and insured for full value. An estimate of repair will be given prior to completion. We must receive a copy of your purchase order via email before non-warranty repair work can commence.

Damaged Goods

Damaged instrumentation should not be returned to Lafayette Instrument prior to a thorough inspection. If a shipment arrives damaged, note damage on delivery bill and have the driver sign it to acknowledge the damage. Contact the delivery service, and they will file an insurance claim. If damage is not detected at the time of delivery, contact the carrier/shipper and request an inspection within 10 days of the original delivery. Please contact the Lafayette Instrument Customer Service Department for repair or replacement of the damaged merchandise.

Limited Warranty

Lafayette Instrument Company warrants equipment to be free of defects in material and workmanship for a period of one year from the date of shipment, except as provided hereinafter. This assumes normal usage under commonly accepted operating parameters and excludes consumable products.

Warranty period for repairs or used instrumentation purchased from Lafayette Instrument is 90 days. Lafayette Instrument Company agrees either to repair or replace, at its sole option and free of part charges to the customer, instrumentation which, under proper and normal conditions of use, proves to be defective within the warranty period. Warranty for any parts of such repaired or replaced instrumentation shall be covered under the same limited warranty and shall have a warranty period of 90 days from the date of shipment or the remainder of the original warranty period whichever is greater. This warranty and remedy are given expressly and in lieu of all other warranties, expressed or implied, of merchantability or fitness for a particular purpose and constitutes the only warranty made by Lafayette Instrument Company.

Lafayette Instrument Company neither assumes nor authorizes any person to assume for it any other liability in connection with the sale, installation, service or use of its instrumentation. Lafayette Instrument Company shall have no liability whatsoever for special, consequential, or punitive damages of any kind from any cause arising out of the sale, installation, service or use of its instrumentation.

All products manufactured by Lafayette Instrument Company are tested and inspected prior to shipment. Upon prompt notification by the Customer, Lafayette Instrument Company will correct any defect in warranted equipment of its manufacture either, at its option, by return of the item to the factory, or shipment of a repaired or replacement part. Lafayette Instrument Company will not be obliged, however, to replace or repair any piece of equipment, which has been abused, improperly installed, altered, damaged, or repaired by others. Defects in equipment do not include decomposition, wear, or damage by chemical action or corrosion, or damage incurred during shipment.

Limited Obligations Covered by this Warranty

1. Shipping charges under warranty are covered only in one direction. The customer is responsible for shipping charges to the factory if return of the part is required.
2. This warranty does not cover damage to components due to improper installation by the customer.
3. Consumable and or expendable items, including but not limited to electrodes, lights, batteries, fuses, O-rings, gaskets, and tubing, are excluded from warranty.
4. Failure by the customer to perform normal and reasonable maintenance on instruments will void warranty claims.
5. If the original invoice for the instrument is issued to a company that is not the company of the end user, and not an authorized Lafayette Instrument Company distributor, then all requests for warranty must be processed through the company that sold the product to the end user, and not directly to Lafayette Instrument Company.